


1/9

FIG. 1

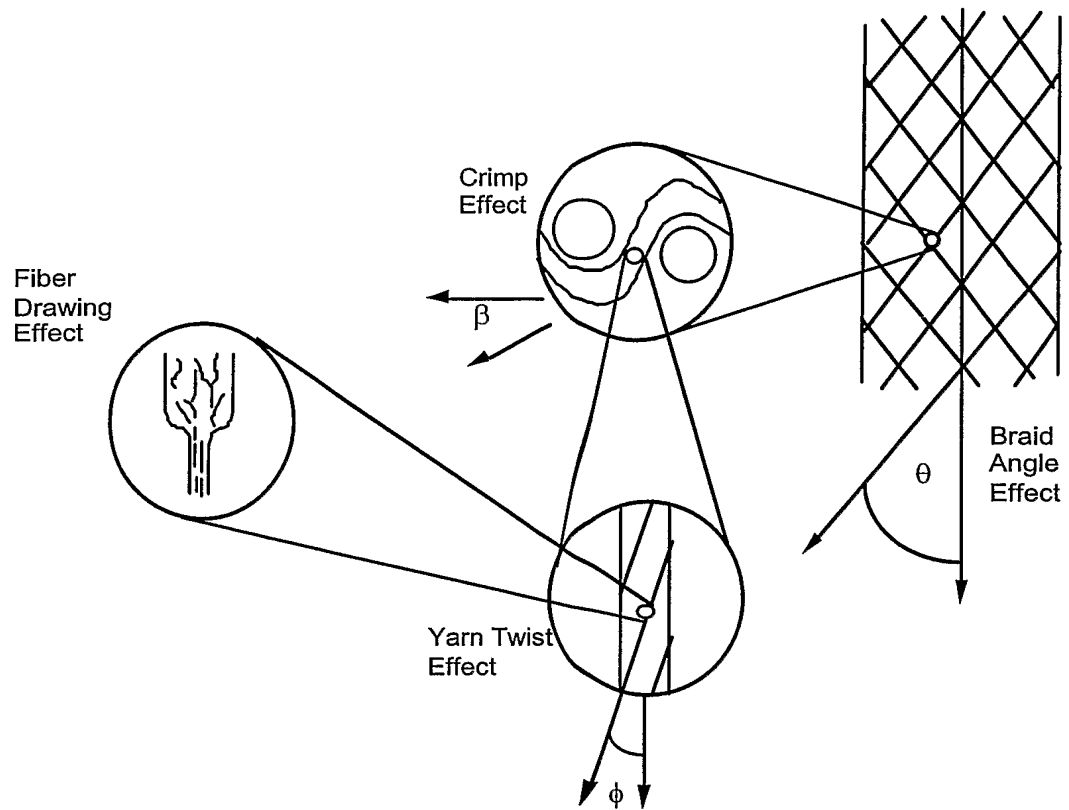

2/9

FIG. 2


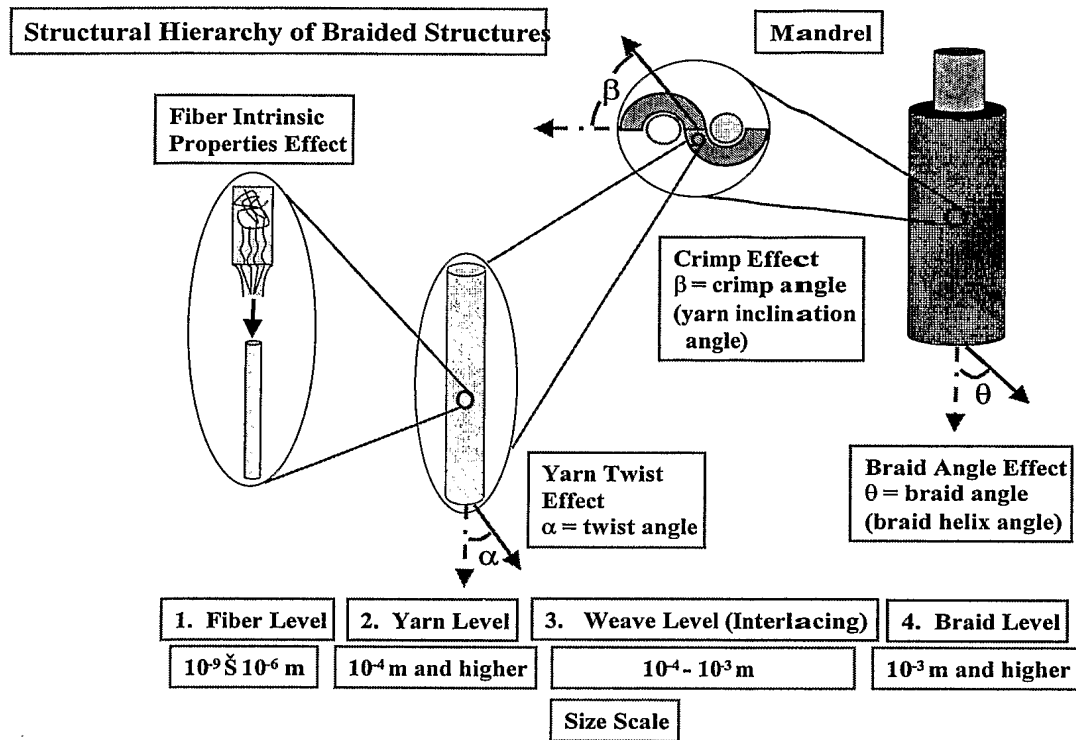


FIG. 3

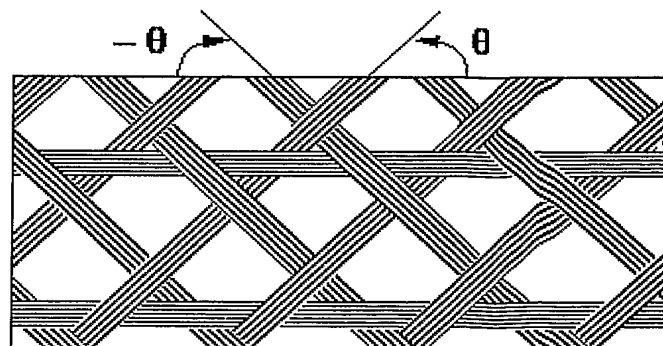

3/9

FIG. 4


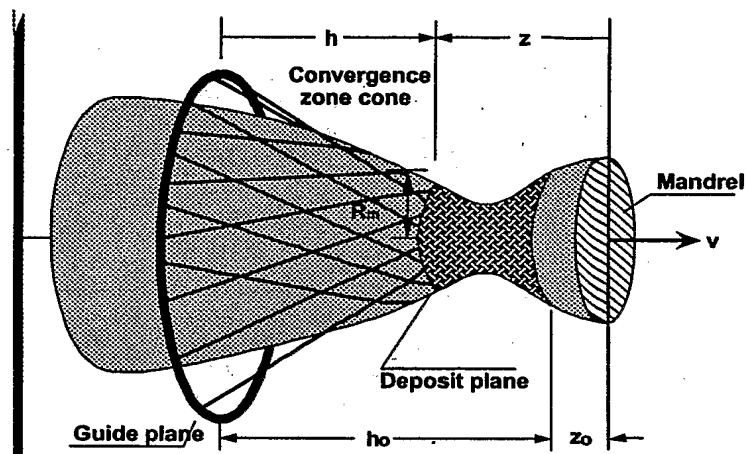


FIG. 5

Process window of fiber volume fraction for braided stent.

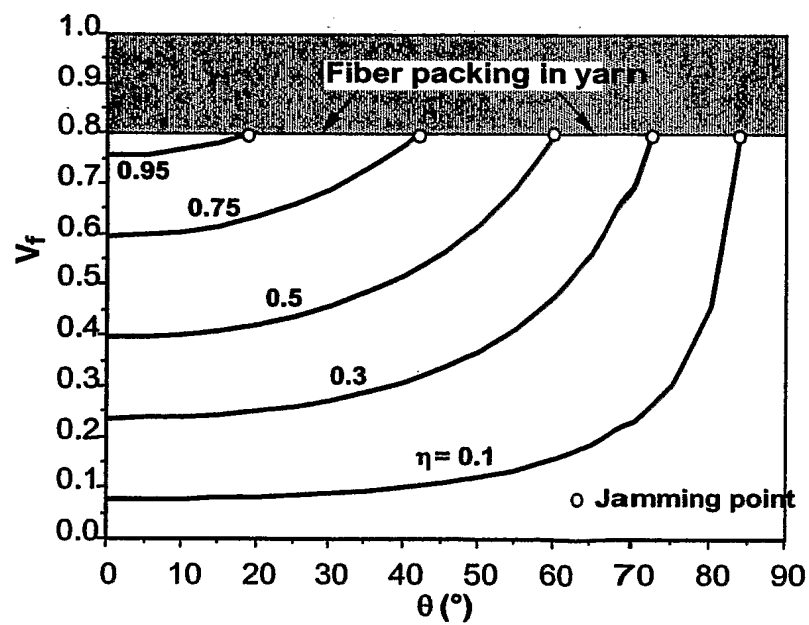

4/9

FIG. 6A

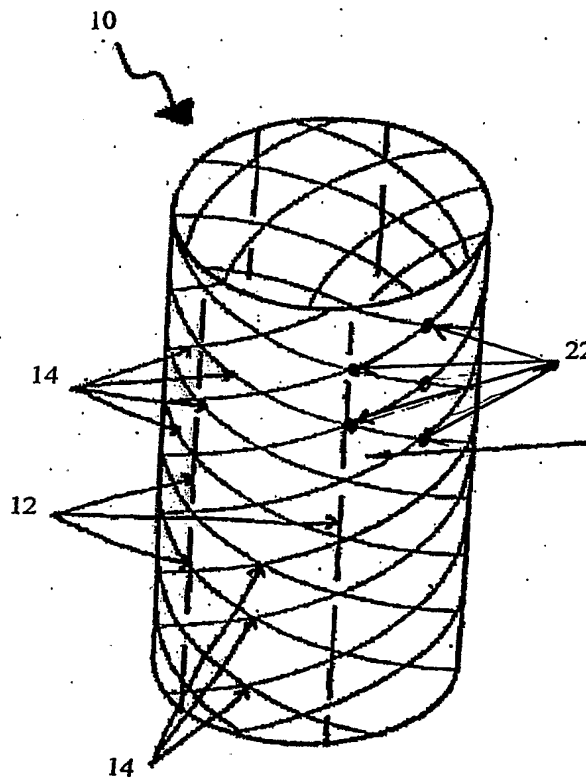


FIG. 6B



FIG. 6C

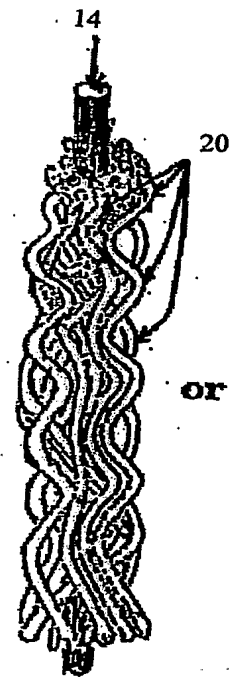


FIG. 6D



5/9

FIG. 7A



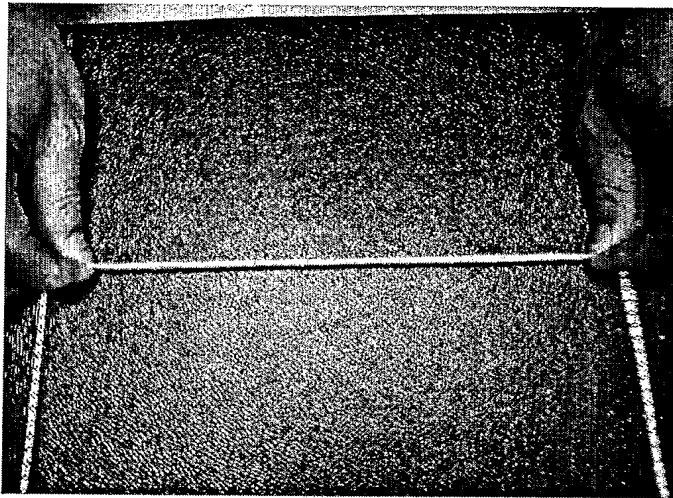


FIG 7B

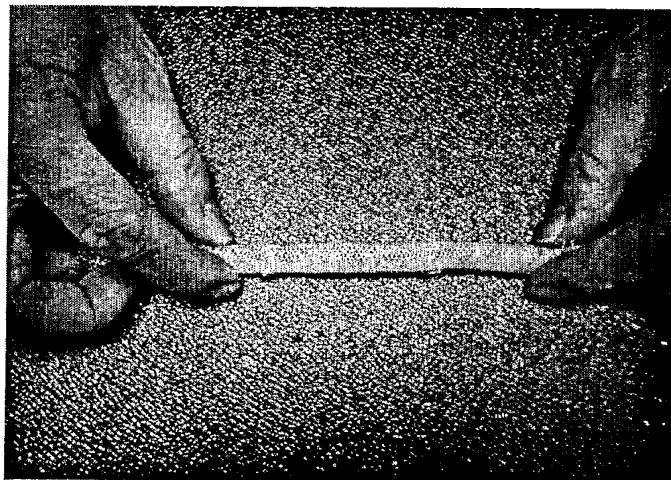

6/9

FIG. 8

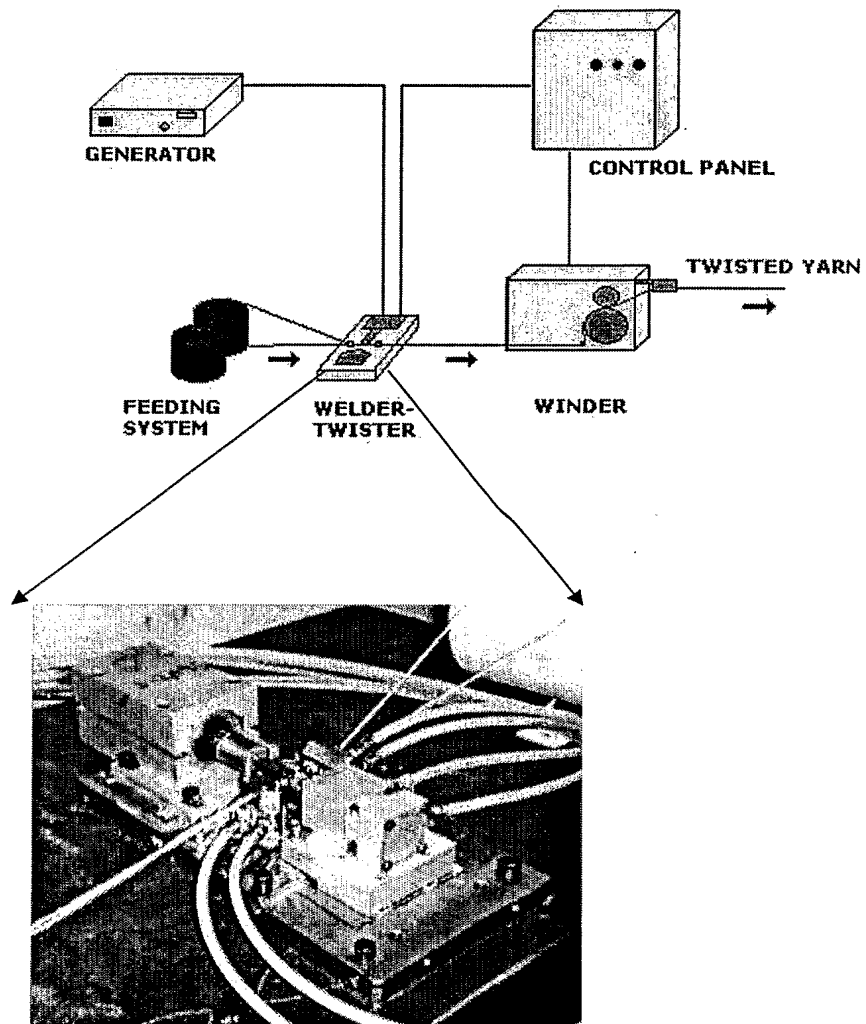

7/9

FIG. 9A



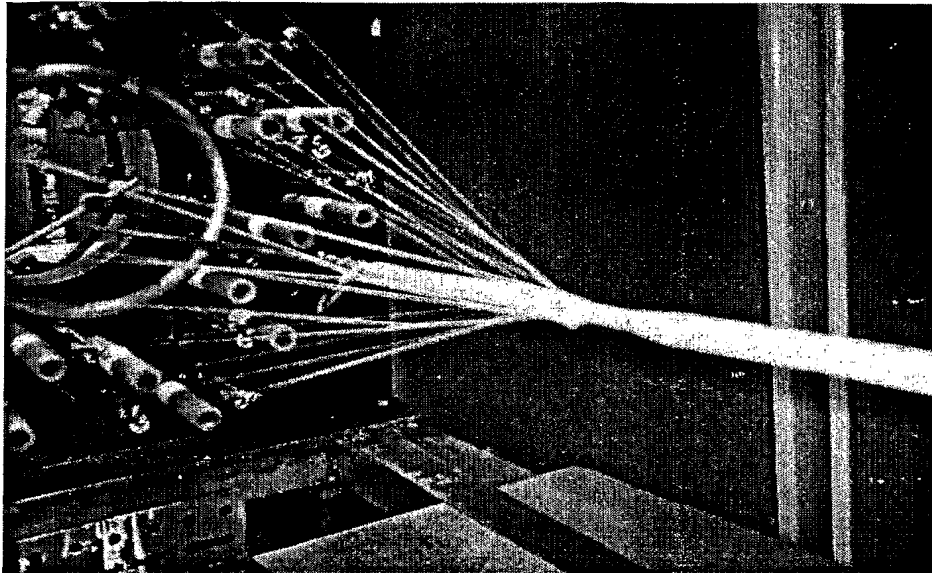


FIG. 9B

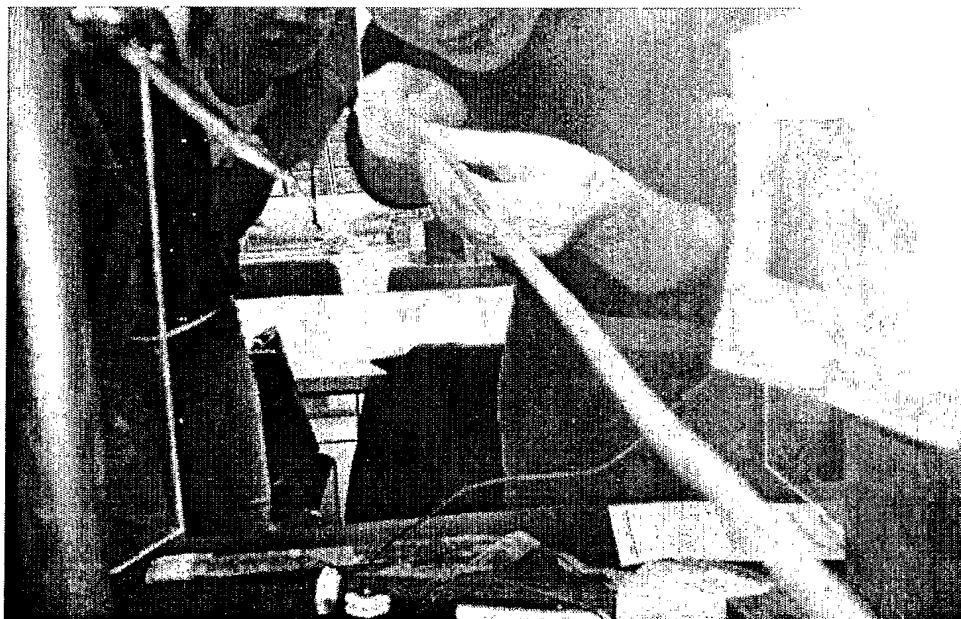

8/9

FIG. 10

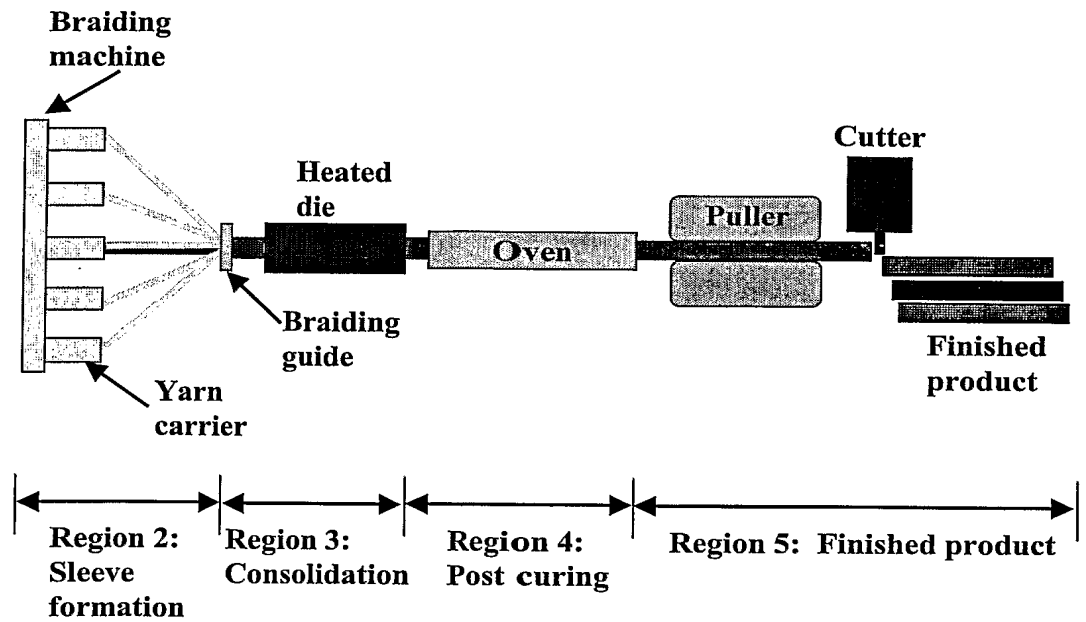



9/9

FIG. 11

